
Our Cord Blood Collection Systems at a glance:







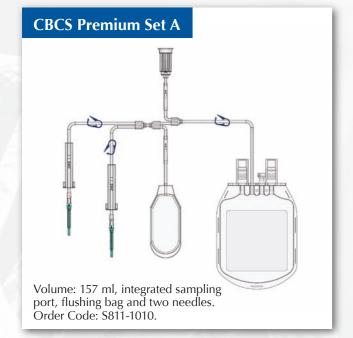

For more information, please contact us:





Bionic Medizintechnik GmbH – a JMS corporation Max-Planck-Str. 21 · D-61381 Friedrichsdorf, Germany Telefon: +49(0)6172-75760 · Fax: +49(0)6172-757610 E-mail: info@bionic-jms.com · www.bionic-jms.com





The efficient and safe Cord Blood Collection System

JMS Cord Blood Collection System – for a safer future

Optimal collection features for easy use

Optimal collection features allow a safe and effective procedure for cord blood collection:

- ➤ Close the clamp near the cannula. Remove the cap and insert the needle into the umbilical cord.
- ▶ Allow the blood collection by placing the collection bag lower than the injection site and opening the clamp.
- Mix blood and anticoagulant gently at several intervals.
- ▶ Close the clamp after the collection is finished.
- Residual blood in the tubing may be flushed by breaking the snap tip to open the optional flushing bag.
- Seal the tube and discard the tubing, flushing bag and needles.

